

MDS Medical AC-DC Adapter

24Volt, 90Watt / MDS-090AAS24 □

090AAS24

Highlights & Features

- Meet DOE Level VI and ErP Lot 7
- Safety Approvals to IEC 60601-1 3.1rd ed. & IEC 62368-1
- Compliant with IEC 60601-1-2 4th Ed. Requirements
- Low touch current (<0.1mA Normal & ,0.3mA single fault)
- Over-Voltage/Load/Temperature & Short Circuit protections
- 1 Million Hours MTBF
- 2 × MOPP isolation
- 3 years warranty

Safety Standards



CB Certified for worldwide use

| | |
|--------------------------------|--|
| Model Number: | MDS-090AAS24 F/B |
| Unit Weight: | 450 grams (16.2 ounces) |
| Dimensions (L x W x H): | 150 x 60 x 35 mm 5.9 x 2.4 x 1.4 in |



General Description

The MDS series of external power supply come with universal AC input at 90Vac to 264Vac. Other features include low touch current, risk management report available and the electric shock protection comply with 2 × MOPP. The MDS series is certified for EMC standards according to EN 55011 for industrial, scientific and medical (ISM) radio-frequency equipment and EN 55032 for Information Technology Equipment (ITE) radio-frequency equipment. In addition, only recognized Japanese capacitors are used.

The MDS series come with both medical and ITE safety approvals including UL/cUL/CCC/CE and CB certification and are fully compliant with RoHS Directive for environmental protection.

Model Information

Medical AC-DC Adapter

| Model Number | Input Voltage Range | Output Voltage | Output Current |
|-----------------|---------------------|----------------|----------------|
| MDS-090AAS24 FA | 90-264Vac | 24Vdc | 3.75A |
| MDS-090AAS24 FE | | | |
| MDS-090AAS24 BA | | | |
| MDS-090AAS24 BE | | | |

Model Numbering

| MDS – | 090 | AAS | 24 | CC Code | |
|-------------------------------|-----------------------------------|-------------|-------------------------|---|---|
| | | | | □ | □ |
| Delta Medical Desktop Adapter | Max wattage in the product series | Family Code | Output Voltage 24 – 24V | Protection Against Shock F: Class I B: Class II with functional Earth | Plug, Molding type and others A: 4Pin Din E: Tuning Fork 5.5x2.5 x 10 |
| Refer to Page 7. | | | | | |

MDS Medical AC-DC Adapter

24Volt, 90Watt / MDS-090AAS24 □

Specifications

Input Ratings / Characteristics

| | |
|------------------------------|--|
| Nominal Input Voltage | 100-240Vac |
| Input Voltage Range | 90-264Vac |
| Nominal Input Frequency | 50-60Hz |
| Input Frequency Range | 47-63Hz |
| Input Current (max.) | 2A @ 115Vac, 1A @ 230Vac |
| Efficiency (typ.) | 90.3%, Reference Fig.1 |
| Average Efficiency (min) | 88% @ 115Vac |
| Standby Power (max.) | 0.21W @ 115Vac |
| Inrush Current (typ.) | 50A @ 115Vac, 100A @ 230Vac |
| Touch Current (max.) | 0.1mA @ 264Vac NC ¹⁾ , 0.3mA @ 264Vac SFC ²⁾ |
| Earth Leakage Current (max.) | 0.1mA @ 264Vac NC ¹⁾ , 0.3mA @ 264Vac SFC ²⁾ |

1) NC: normal condition

2) SFC: single fault condition

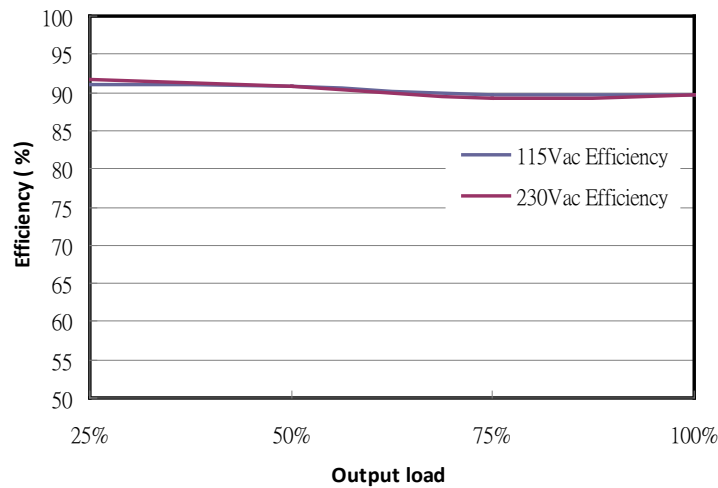



Fig.1 Efficiency versus output load

Output Ratings / Characteristics

| | |
|---|--|
| Nominal Output Voltage | 24Vdc |
| Total Regulation | ±5% |
| Output Current | 3.75A |
| Output Power | 90W |
| Line Regulation (max) | ±0.5% |
| Load Regulation (max) | ±4.5% |
| Ripple & Noise (typ.) | 94.4mV pk-pk @ Full load, Reference Fig. 2 |
| Start-up Time (max) | 3000ms |
| Hold-up Time (min) | 20ms @ 115Vac&230Vac |
| Dynamic Response (Overshoot & Undershoot O/P Voltage) | ±5% @ 50-100% load |

MDS Medical AC-DC Adapter

24Volt, 90Watt / MDS-090AAS24 □

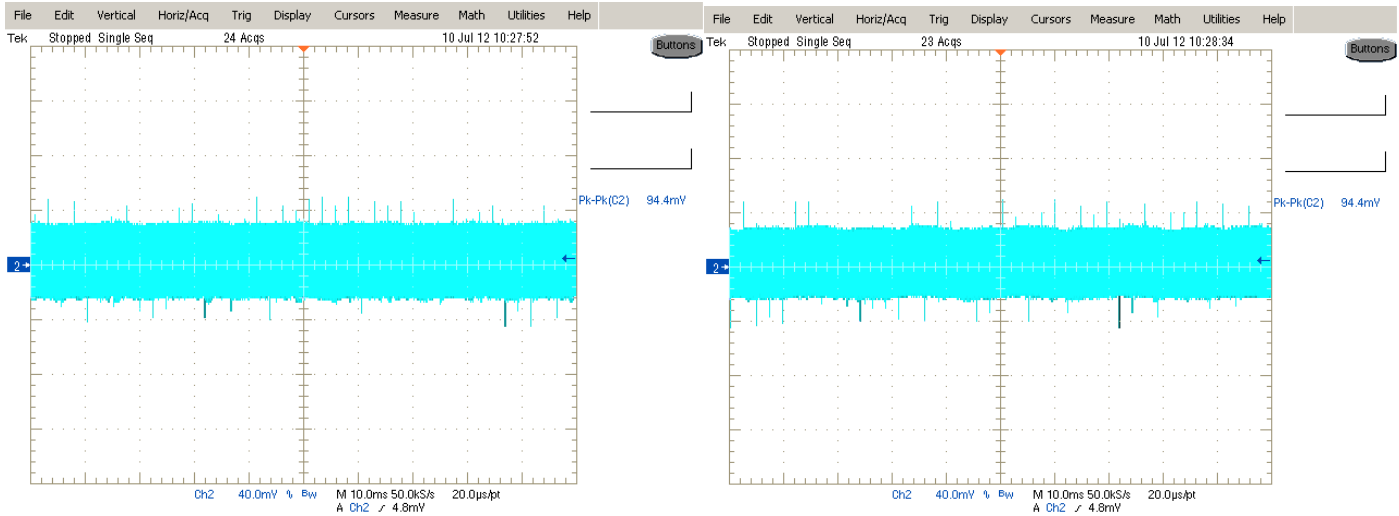


(a) 115V

(b) 230V

Fig. 2 Ripple & Noise example, 20MHz BW

Ripple & Noise measurement circuit

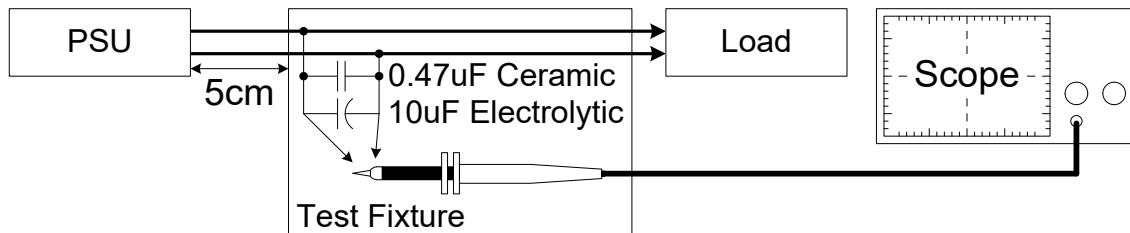

Mechanical

| | |
|------------------------|--|
| Case Chassis | PC |
| Case Cover | PC |
| Dimensions (L x W x H) | 150 x 60 x 35 mm (5.9 x 2.4 x 1.4 in) |
| Unit Weight | 450grams (16.2ounces) |
| Indicator | NA |
| Cooling System | NA |
| Terminal | Input: C14 socket Output: 4pin Din / Tuning fork type |

Environment

| | | |
|-----------------------------|-----------|--|
| Surrounding Air Temperature | Operating | 0°C to +40°C |
| | Storage | -40°C to +85°C |
| Operating Humidity | | 10-95% RH (Non-Condensing) |
| Operating Altitude | | 3,000 meters (9842.52 feet) |
| Shock Test (Non-Operating) | | 50G, 11ms, 3 shocks for each direction |
| Vibration (Non-Operating) | | 5-500Hz, 2.09Grms, 20 minute for each three axis |

MDS Medical AC-DC Adapter

24Volt, 90Watt / MDS-090AAS24 □

Protections

| | |
|---------------------------------|--|
| Overvoltage (max.) | 150%, Latch Mode |
| Over load / Over current (max.) | 130% of rated load current, Hiccup Mode, (Non-Latching, Auto-Recovery) |
| Over Temperature | Hiccup Mode, (Non-Latching, Auto-Recovery) |
| Short Circuit | Hiccup Mode, (Non-Latching, Auto-Recovery) |
| Protection Against Shock | Class I for F series |
| | Class II with functional earth for B series |

Reliability Data

| | |
|-------------|--------------------------------------|
| MTBF (typ.) | 1 Million based on Telecordia SR-332 |
|-------------|--------------------------------------|

Safety Standards / Directives

| | | |
|--------------------|--|----------|
| Medical Safety | IEC60601-1 3 rd and 3.1 rd edition CB report IEC60601-1 edition 3.1rd (2012), EN60601-1 (2006) + A11 + A1 + A12, CAN/CSA-C22.2 NO. 60601-1:14, ANSI/AAMI ES60601-1:2005/(R)2012 | |
| ITE Safety | IEC60950-1 (Ed.2,2005), IEC62368-1, GB4943.1-2011, GB9254-2008, GB17625.1-2003 | |
| CE | MDD Directive 93/42/EEC | |
| Galvanic Isolation | Input to Output | 4000 Vac |
| | Input to Ground | 1500 Vac |
| | Output to Ground | 500 Vac |

MDS Medical AC-DC Adapter

24Volt, 90Watt / MDS-090AAS24 □

EMC (Compliant with IEC 60601-1-2 4th Ed. Requirements)

| | | |
|-----------------------------------|---------------|---|
| EMC / Emissions | | EN55011/EN55032, FCC Title 47:Class B |
| Harmonic Current Emissions | IEC61000-3-2 | Meet Class A limit |
| Immunity to | | |
| Voltage Flicker | IEC61000-3-3 | |
| Electrostatic Discharge | IEC61000-4-2 | Level 4 Criteria A ¹⁾ Air Discharge: 15kV Contact Discharge: 8kV |
| Radiated Field | IEC61000-4-3 | Criteria B ²⁾ 80MHz-2700MHz, 10V/m AM modulation 385MHz-5785MHz, 28V/m Pulse mode and other modulation |
| Electrical Fast Transient / Burst | IEC61000-4-4 | Level 3 Criteria A ¹⁾ :2kV |
| Surge | IEC61000-4-5 | Level 3 Criteria A ¹⁾ Common Mode ³⁾ : 2kV Differential Mode ⁴⁾ : 1kV |
| Conducted | IEC61000-4-6 | Level 2 Criteria A ¹⁾ 150kHz-80MHz, 3Vrms, 6Vrms at ISM bands and Amateur radio bands |
| Power Frequency Magnetic Fields | IEC61000-4-8 | Criteria A ¹⁾ Magnetic field strength 30A/m |
| Voltage Dips | IEC61000-4-11 | Criteria A ¹⁾ 0% U _T , 0.5 cycle (10ms) , 0°/45°/90°/135°/180°/225°/270°/315°/360° Criteria A ¹⁾ 0% U _T , 1 cycle (20ms), 0° Criteria B ²⁾ 70% U _T , 25 cycle (500ms), 0° Criteria B ²⁾ 0% U _T , 250 cycle (5000ms), 0° |

1) Criteria A: Normal performance within the specification limits

2) Criteria B: Output out of regulation, or shuts down during test. Automatically restore to normal operation after test.


3) Asymmetrical: Common mode (Line to earth)

4) Symmetrical: Differential mode (Line to line)

MDS Medical AC-DC Adapter


24Volt, 90Watt / MDS-090AAS24 □

Block Diagram

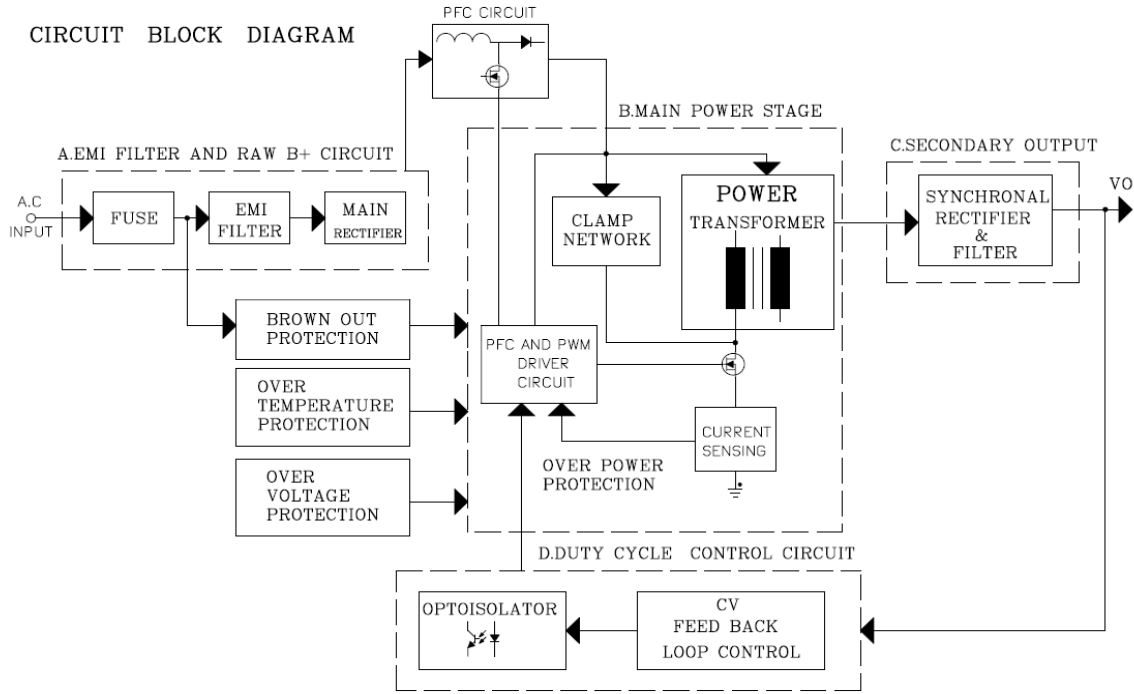

Dimensions:

W x L x H: 60.0x 150.0 x 35.0 mm

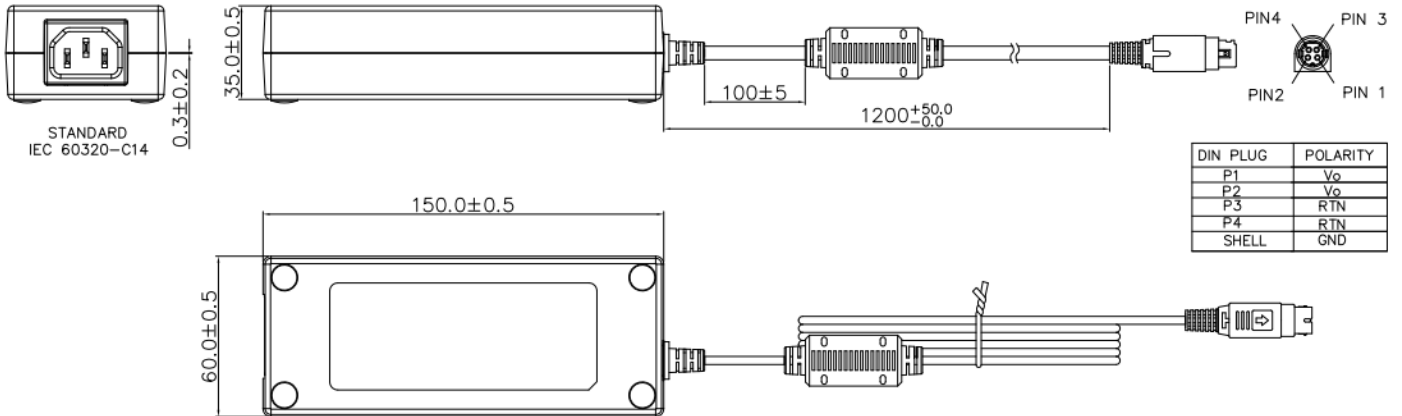



Notes:
Dimension are in mm

| Item | Device Description |
|------|--------------------|
| 1 | Cover |
| 2 | Chassis |
| 3 | Power Cord |
| 4 | Socket |

MDS Medical AC-DC Adapter

24Volt, 90Watt / MDS-090AAS24 □

DC Output Plug:
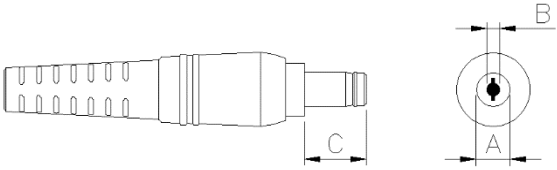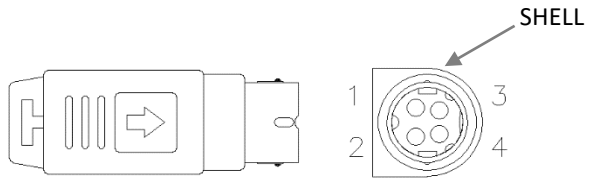
| Turing Fork | CC Code | Cable Length | A | B | C |
|---|---------|--------------|----------------|-----|----|
| | | | OD | ID | L |
|  | BE | 1.2m | 5.5 | 2.5 | 10 |
| | FE | 1.2m | 5.5 | 2.5 | 10 |
| Mini DIN 4 Pins with Lock (Male) | CC Code | Cable Length | Pin Assignment | | |
|  <p>KYCON KPPX-4P Equivalent</p> | BA | 1.2m | 1 | +Vo | |
| | | | 2 | +Vo | |
| | | | 3 | -Vo | |
| | | | 4 | -Vo | |
| | | | Shell | - | |
| | FA | 1.2m | 1 | +Vo | |
| | | | 2 | +Vo | |
| | | | 3 | -Vo | |
| | | | 4 | -Vo | |
| | | | Shell | - | |

MDS Medical AC-DC Adapter

24Volt, 90Watt / MDS-090AAS24 □

Functions

Start-up Time

The time required for the output voltage (V_o) to reach 90% of its set value, after the input AC voltage is applied.


Rise Time

The time required for the output voltage (V_o) to change from 10% to 90% of its steady state value.

Hold-up Time

Hold up time is the time when the AC input collapses and output voltage retains regulation for a certain period of time. The time required for the output to reach 95% of its set value, after the input voltage is removed.

■ Graph illustrating the Start-up Time, Rise Time, and Hold-up Time

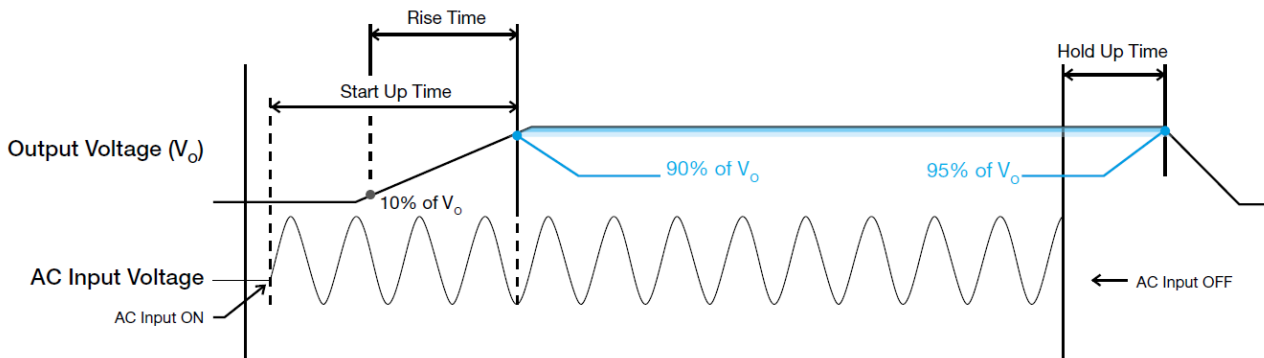


MDS Medical AC-DC Adapter

24Volt, 90Watt / MDS-090AAS24 □


Dynamic Response

The power supply output voltage will remain within $\pm 5\%$ of its steady state value, when subjected to a dynamic load change from 50 to 100% of its rated current.

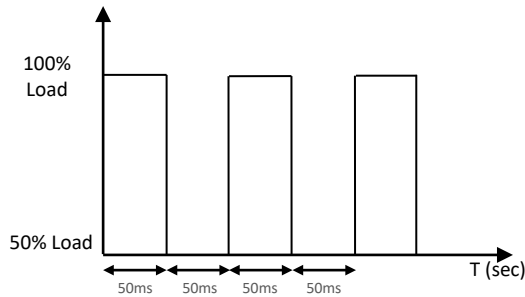

Inrush Current

Inrush current is the input current that occurs when the input voltage is first applied. For AC input voltages, the maximum peak value of inrush current will occur during the first half cycle of the applied AC voltage. This peak value decreases exponentially during subsequent cycles of AC voltage.

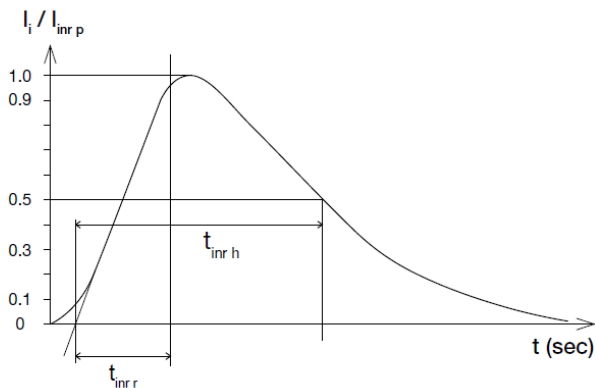

Overvoltage Protection


The power supply's overvoltage circuit will be activated when its internal feedback circuit fails. The output voltage shall not exceed its specifications defined on Page 4 under "Protections". Power supply will latch off, and require removal/re-application of input AC voltage in order to restart.

Short Circuit Protection

The power supply's output OLP/OCP function also provides protection against short circuits. When a short circuit is applied, the output current will operate in "Hiccup mode", as shown in the illustration in the OLP/OCP section on this page. The power supply will return to normal operation after the short circuit is removed.

Overload & Over current Protections

The power supply's Overload (OLP) and Over current (OCP) Protections will be activated when output current is between 110% and 130% of I_o (Max load). Upon such an occurrence, V_o will start to drop. Once the power supply has reached its maximum power limit, the protection will be activated, and the power supply will go into "Hiccup mode" (Auto-Recovery). The power supply will recover once the fault condition causing the OLP and OCP is removed and I_o is back within the specified limit.

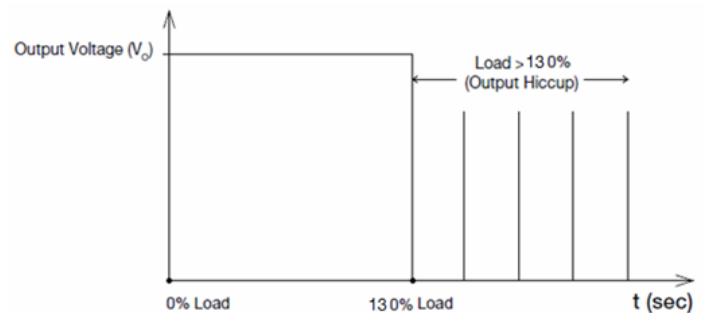

Additionally, if the I_o is $< 130\%$ but $> 110\%$ for a prolonged period of time (depending on the load), the Over Temperature Protection (OTP) will be activated due to high temperature on critical components. The power supply will then go into hiccup mode until the fault is removed; and, the input voltage is removed, then reapplied.

Over Temperature Protection

As mentioned above, the power supply also has Over Temperature Protection (OTP). This is activated when the overload condition persists for an extended duration and the output current is below the overload trigger point but $> 100\%$ load. In the event of a higher operating condition at 100% load, the power supply will run into OTP when the surrounding air temperature is higher than the operating temperature. When activated, the output voltage will go into hiccup mode until the input voltage is removed; then, reapplied, and the surrounding air temperature drops to its normal operating temperature.

MDS Medical AC-DC Adapter

24Volt, 90Watt / MDS-090AAS24 □

Certificate



Delta has been certified as meeting the requirement of ISO 13485: 2003 and EN ISO 13485:2012 for the design and manufacture of switching power supply and adaptor for medical device.



In addition to a UL Total Certification Program (TCP) approved client laboratory for IEC62368-1. Delta also has participated UL Client Test Data Program (CDTP) for IEC 60601



Meet DOE Level VI and ErP Lot 7 Efficiency Requirement

Attention

Delta provides all information in the datasheets on an "AS IS" basis and does not offer any kind of warranty through the information for using the product. In the event of any discrepancy between the information in the catalog and datasheets, the datasheets shall prevail (please refer to www.DeltaPSU.com for the latest datasheets information). Delta shall have no liability of indemnification for any claim or action arising from any error for the provided information in the datasheets. Customer shall take its responsibility for evaluation of using the product before placing an order with Delta.

Delta reserves the right to make changes to the information described in the datasheets without notice.